



Gas Analysis

WWW.MKSINSTITUTE.COM

MultiGas™ 2030 ON-LINE GAS ANALYSIS

The MultiGas 2030 is an FTIR based analyzer capable of ppb to ppm sensitivity for multiple gas species in a variety of applications, such as stack emissions monitoring, process monitoring, ambient air monitoring, purity monitoring, and selective catalytic reduction performance monitoring. The MultiGas 2030 can perform analysis in gas streams that contain up to 30% water, and can simultaneously analyze and display more than 30 gases. With permanently stored calibration spectra, the need for costly gas cylinders is reduced. In addition, operators will find the robust, fully automated MultiGas 2030 easy to operate and maintain.

The MultiGas 2030 Analyzer is composed of a 2102 Process FTIR Spectrometer, our patented, high-optical-throughput sampling cell, applications-specific analysis software, and an instrument independent quantitative spectral library. The MultiGas 2030 collects high-resolution infrared spectra which are analyzed using the quantitative spectral library. This provides an accurate, highly sensitive measurement of most gases and vapors.


Features & Benefits

- 10-100 ppb sensitivity for many toxic gases
 - Including VOCs, acids, bases, hydrides, and PFCs
 - In effluent streams that contain up to 30% water
- Easily transportable from site to site, with set up time in minutes
- Simultaneous analysis and display of more than 30 gases
- Permanent calibration spectra reduces the need for costly gas cylinders
- Gas line heater maintains temperature before the sample enters gas cell
- Patented, linearized detector response assures all instruments maintain the same calibration
- Frequency and resolution diagnostics ensure constant calibration
- Provides automatic temperature and pressure compensation to ensure accurate analysis
- User-friendly software enables simple operation by minimally trained personnel

Applications

- Stack monitoring (environmental compliance)
- Process monitoring, development and optimization
- Ambient air analysis (industrial hygiene)
- Bulk gas purity analysis
- Combustion emissions monitoring
- SCR - selective catalytic reduction



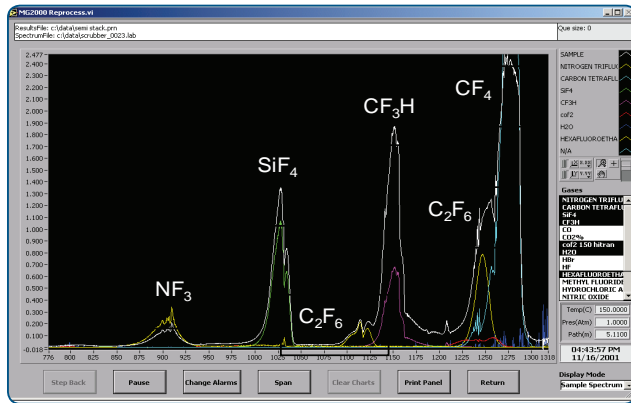

IR Spectrum of Semiconductor Stack: Sample (white), Calibrations (color). The MultiGas 2030 can speciate (differentiate) similar molecules simultaneously.

Designed specifically for process and environmental monitoring, the 2102 Process FTIR Spectrometer is compact and rugged. Capable of operating at spectral resolutions up to 0.5 cm^{-1} , it is the fastest, most sensitive and stable process FTIR available. In addition, it can operate in hostile environments with a high degree of immunity to vibration and temperature changes. An advanced, high-speed data processing system is standard, and provides low-noise infrared spectra for analysis.



2102 Process FTIR Spectrometer

This spectrometer is coupled to a patented low volume (200 mL) multi-pass gas cell with a 5.11 meter effective pathlength. The patented design of this cell incorporates aspheric, aberration-correcting mirrors which provide more than twice the optical throughput of a conventional multi-pass gas cell. Alternatively, a single-pass gas cell can be used for corrosive gases or strongly-absorbing gases at high concentrations. Either cell can be operated from ambient temperature to 150°C .




The 5.11m pathlength, 200 mL volume, long path gas cell measures $8\text{-}1/2" \times 2" \times 3\text{-}1/2"$, and uses a patented aberration correcting optics for maximum sensitivity.


Spectral Analysis

The MultiGas analyzer features robust quantitative analysis software, which can analyze and report concentrations for dozens of compounds simultaneously. The software, which operates on a personal computer, performs automatic corrections for gas temperature and pressure variations, which are measured directly by the analyzer. Samples can be acquired and analyzed in less than a second, making transient analysis possible.

During data collection the MultiGas software continuously acquires and processes spectra while computing the concentrations of the gases that are selected in the setup. Display formats include concentration histories in graphical and tabular formats, the measured spectrum and spectral residuals. The residual spectrum can be utilized to visually determine error in the analysis, making QA/QC checking easy and straight forward to accomplish. The spectral residuals represent the "left-over" spectral information once all the reference spectra have been accounted for. Once spectra have been collected and saved, these spectra may be reprocessed at any time using the same or different calibration sets.

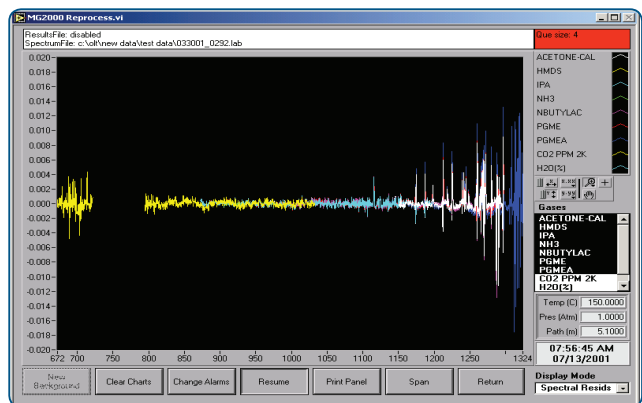

Residual Spectra: Calibration Subtracted from Sample Demonstrates Analysis Quality

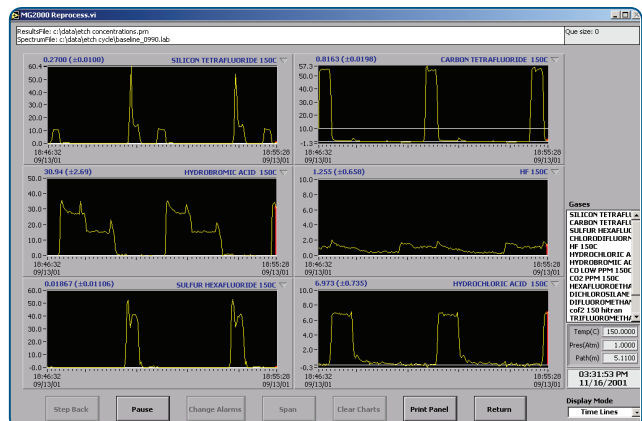


Time Lines from Semiconductor Process



Instrument Independent Calibration

The MultiGas software features multi-point calibration curves that provide a dynamic range up to 9 orders of magnitude (ppb to 100%). Calibrations for many species are provided with the instrument, and additional calibrations can be generated by the user from gases of known concentration. Utilities in the MultiGas software verify the performance of each instrument, which allows a calibration generated on one MultiGas to be used on any other MultiGas without alteration.

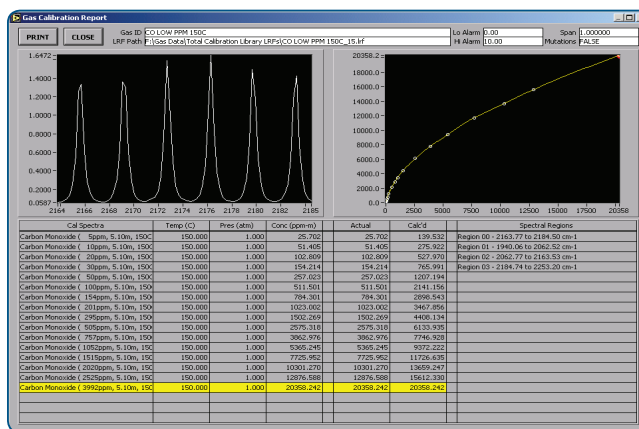

Graphical User Interface for Calibration

Specifications

Analyzer

Measurement Technique

FTIR Spectrometry

Gases and Vapors Measurable

Most molecules except for N₂, H₂, and O₂

Ranges

Concentration setting between 10ppb and 100% full scale

FTIR

2102 Process FTIR

Spectral Resolution

0.5 – 128cm⁻¹

Scan Speed

1 scan/sec @ 0.5cm⁻¹

Scan Time

1-300 sec

Infrared Source

Silicon Carbide @ 1200°C

Reference Laser

Helium Neon (15798.2cm⁻¹)

Detector

LN₂-cooled MCT; TE-cooled MCT

Purge Pressure

20 psig (1.5 bar) max.

Spectrometer Purge Flow

0.2 L/min of dry nitrogen or CO₂ free clean dry air with dewpoints below -70°C

Optics Purge Flow

0.2 L/min of dry nitrogen or CO₂ free clean dry air with dewpoints below -70°C

Pressure Transducer

MKS Baratron®

Purge Connection

Swagelok® quick connect

Computer Requirements

Desktop or notebook Intel Pentium® PC under Microsoft® Windows® XP display (1024 x 768)

Recommended

Intel Pentium III, 850 MHz, Microsoft Windows XP, 256 MB

Communications

RJ-45 cross-over Ethernet

Output Options

XML, analog, AK, others (please inquire)

Dimensions

17.5"W x 12.5"H x 25.5"D

Installation

19" rack mount chassis

Power

120 or 240 VAC, 50/60 Hz, 3 amps

Weight

110 lbs. (50 kg)



Specifications (continued)

Sampling Parameters

Sample Temperature	Ambient to 200°C (calibration temperature dependant)
Sample Flow	0.2 – 10 L/min
Sample Pressure	0.01 – 4 atm (calibration pressure dependant)

Gas Cell

Construction	Nickel coated Al; Welded 316 stainless steel optional
Fittings	¼" Swagelok®, ¼" VCR®
Tubing	Heated ¼" stainless steel
Mirrors	Nickel plated aluminum substrate, with rugged gold coating
Windows	KBr; CaF ₂ (others available)
O-rings	Viton® (others available)

Detection Limits

Low-level detection limits for the 5.11 meter gas cell and a mercury-cadmium-telluride (MCT) detector at 0.5 cm⁻¹ resolution for typical gases in the absence of interfering species are as follows:

Name	Formula	Lowest Detectable Limit with 20/20™ Cell and 5 min Measurement	Lowest Detectable Limit with 20/20™ Cell and 1 sec Measurement
Ammonia	NH ₃	30ppb	0.5ppm
Carbon Dioxide	CO ₂	12ppb	0.2ppm
Carbon Monoxide	CO	72ppb	1.2ppm
Formaldehyde	H ₂ CO	36ppb	0.6ppm
Hydrogen Chloride	HCl	87ppb	1.5ppm
Hydrofluoric Acid	HF	12ppb	0.2ppm
Methane	CH ₄	36ppb	0.6ppm
Nitrogen Dioxide	NO ₂	24ppb	0.4ppm
Nitric Oxide	NO	210ppb	3.6ppm
Nitrogen Trifluoride	NF ₃	30ppb	0.5ppm
Silicon Tetrafluoride	SiF ₄	10ppb	0.15ppm
Sulfur Dioxide	SO ₂	36ppb	0.6ppm
Tetrafluoromethane	CF ₄	2.5ppb	40ppb
Xylenes	C ₈ H ₁₀	60ppb	1.0ppm

Ordering Information

Please contact your local MKS office for price and availability information.



MKS Global Headquarters

2 Tech Drive, Suite 201
Andover, MA 01810
Tel: 978.645.5500
Tel: 800.227.8766 (in USA)
Web: www.mksinst.com

Gas Analysis/FTIR

651 Lowell Street
Methuen, MA 01844
Tel: 978.645.5500
Tel: 800.227.8766 (in USA)